

# Human CD3E-coupled Magnetic Beads

Cat.No. MBS-K026

## ■ Product Description

The Human CD3E-coupled Magnetic Beads is produced by coupling biotinylated CD3E protein to streptavidin-conjugated magnetic beads. This takes advantage of the extraordinarily strong interaction between biotin and streptavidin, meaning the protein is effectively bound irreversibly. These characters enable the beads to achieve a high yield and low non-specific binding in protein separation.

These beads can be utilized for a wide array of applications, including bio panning, immunocapture, flow cytometry, etc. This product offers a convenient and efficient way to capture proteins of interest in solution. All you need is a magnet.

## ■ Protein Information

**Protein Description:** Biotinylated Human CD3 epsilon, His, Avi tag

**Expression platform:** HEK293 cells

**Calculated MW:** 15.45 kDa

**AA range:** AA Asp 23 - Asp 126 (Accession # P07766-1)

## ■ Beads Information

**Bead size:** 2 mg/5 mg

**Particle size:** 2  $\mu$ m

**Magnetism:** Superparamagnetic

**Number of beads/mg:**  $1 \times 10^8$  beads/mg

**Amount of protein coupled:** 265 pmol (4.1  $\mu$ g) CD3E/mg


Beads

## ■ Storage

This product is stable for 1 year when stored at  $-20$  °C.

Please avoid more than 3 freeze-thaw cycles once reconstitution, immediate use after reconstitution is highly recommended.

## ■ Sample Data

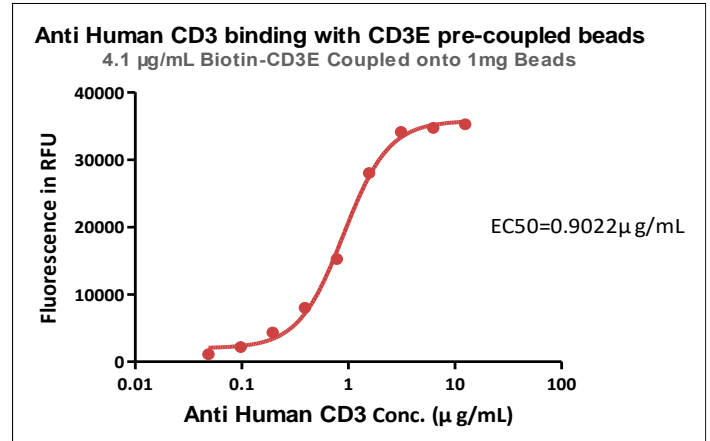

Immobilized 4.1  $\mu$ g CD3E/1mg beads can bind the Anti Human CD3 antibody (Cat. No. MBS-K026) with an EC50 of 0.9022  $\mu$ g/mL (QC tested).

## ■ General guidelines

Use a magnetic separator that is suitable for your equipment and application. Allow the beads to separate for at least 1 minute before removing supernatant. The beads are dense and will tend to settle very quickly. Be sure that any bead mixture is homogenous before aliquoting.

Before any experiment, it is necessary to wash the magnetic beads to remove trehalose from the formulation buffer and change the buffer to your Assay/Washing Buffer.

1. Place the tube with reconstituted beads on a magnetic separator for 2 min. Remove the supernatant.
2. Remove the tube from the magnetic separator and resuspend the pelleted beads in equal volume (or at least 1000 $\mu$ L) of Assay/Washing Buffer. Mix by vortex for approximately 10 sec.
3. Place the tube on the magnetic separator for 2 min. Remove the supernatant.
4. Wash the beads for three times in total by repeating steps 2 and 3.

## ■ Binding assay

Below is a suggested antibody capture protocol for your reference.

1. Reconstitute and wash the magnetic beads according to the Certificate of Analysis. Immediate use is strongly recommended.
2. Add 1 mL Assay/Washing Buffer per mg beads to resuspend the beads. The most common Assay/Washing Buffer is PBS, pH 7.3 with 0.05% Tween-20. Optionally, you may add 0.05% BSA. When assaying a serum sample, please choose a Special Assay/Blocking Buffer (Cat. No. MB-12) to minimize the background signal.
3. Sample Dilution: Dilute your antibody of interest from 12.5µg/mL to 0.012µg/mL in Assay Buffer.
4. Add 100 µL beads to each tube or plate well. Place the beads on the magnetic separator for 1-2 min. Remove the supernatant.
5. Add 100 µL diluted sample to the pelleted beads, and mix the beads with samples by mixer. Add 100 µL Assay Buffer as a blank control into wells containing the beads.
6. Cover the tubes on a rotator or place the plate on a plate mixer and incubate for 60 minutes at room temperature. Alternatively, rotate overnight at 4°C.
7. Place the tube/plate on the magnetic separator for 2 min. Remove the supernatant.
8. Remove the tube/plate from the magnetic separator and resuspend the pelleted beads in 200 µL Assay/Washing Buffer by a vortex.
9. Wash the beads for a total of 4 times by repeating steps 7–8. After the last wash, remove the supernatant.
10. Dilute your Secondary Antibody in Assay buffer. Add 100µL secondary antibody (at an appropriate dilution ratio) to the beads. We recommend PE anti-Human IgG Fc (Biolegend, Cat. No. 409304) at 1:200 to detect your human IgG antibody samples. Any other fluorescent-labeled secondary antibody is appropriate.

11. Place the tubes on a rotator or place the plate on a plate mixer, and incubate for 60 minutes at room temperature. Cover with foil to avoid photobleaching.

12. Repeat steps 7-8 for a total of four washes with Assay/Washing buffer. After the last wash, remove the supernatant.

13. Resuspend the beads by adding 100 µL Assay/Washing Buffer to the beads.

14. Transfer the 100µL beads into a 96-well black plate that is compatible with your plate reader. Keep the beads well suspended.

15. Read the plate at excitation 488 nm/emission 575 nm on a plate reader within 10 min (Avoid precipitation of the beads).

## ■ Important Note

This product is for research use only and not intended for therapeutic or *in vivo* diagnostic use.

## ■ Contact Information

If you have any questions, please contact our technical support team at: [TechSupport@acrobiosystems.com](mailto:TechSupport@acrobiosystems.com)